

Protocol of sensor [28-030197941e15]

Determination of temperature homogeneity in real time.

Device:		Customer:	TEST CHAIN
Type:		Address:	Somewhere 1
Serial Num:		Location:	Shop
Inventory Num:		Server:	TemPiV1-E2C828
Producer:		Sensor Name:	Sklad2


Used Digital Thermometer Sensor

Name	Serial Number	Measuring range	Producer	Scale division
DS18B20	28-030197941e15	-55 'C to 125 'C	DALLAS	0,001 'C

General measurement information

Number of measured values	718
Controlled temperature value	23 - 26
Measurement interval	*/2 minute
Initial measurement time	00:00:08
Final measurement time	23:54:10
Number of alarm states per period	18
Temperature Min	21.125
Temperature Max	25.187
Temperature Average	23.7053
Temperature variance	4.062

Daily course (in 24 hours)

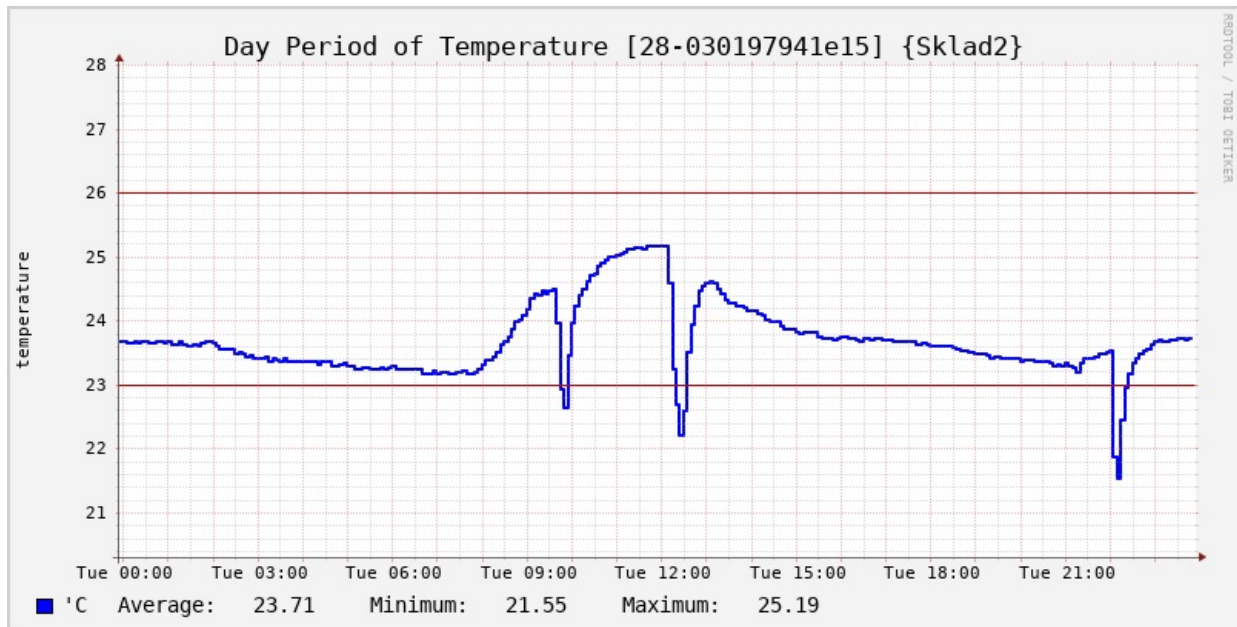

Date: 01 Dec 2020 23:54:01

Signature: